

1/4

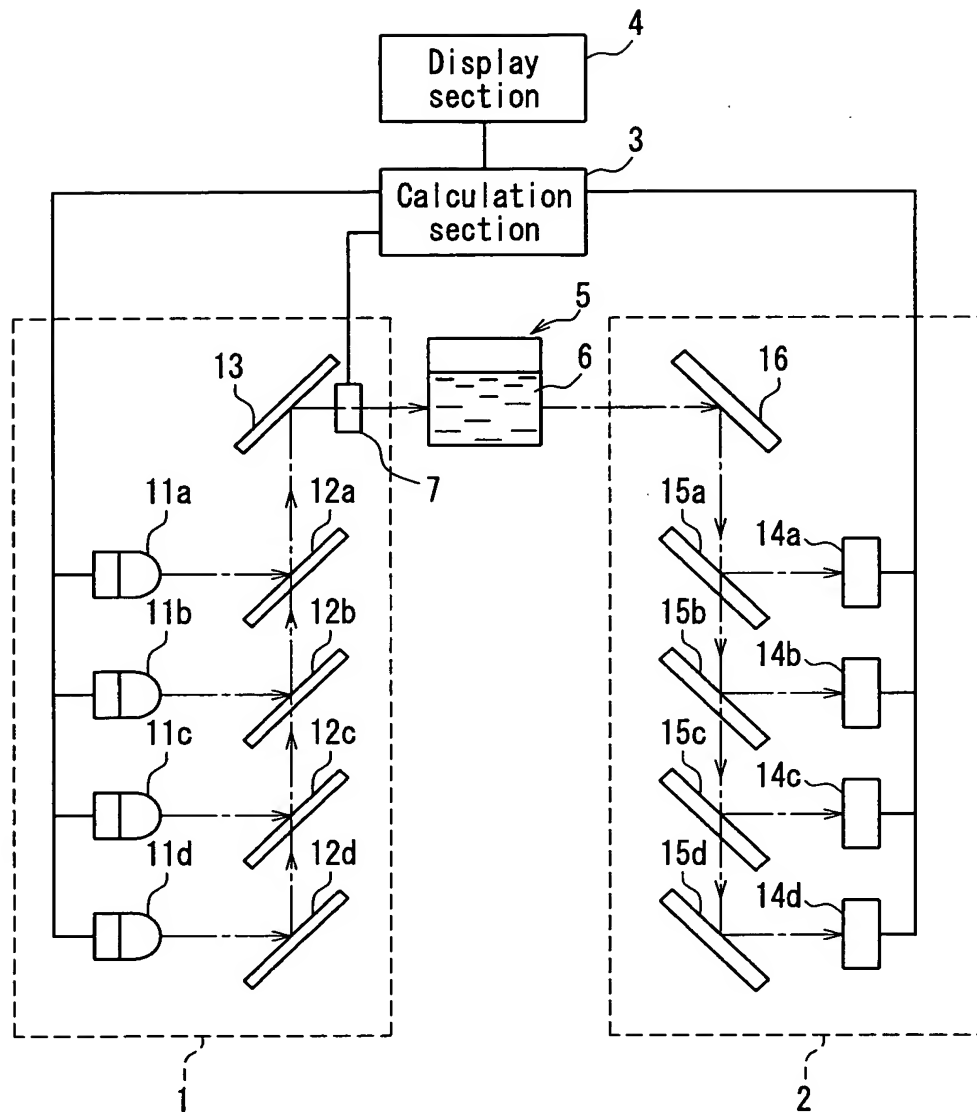


FIG. 1

2/4

Fluorescence measuring process

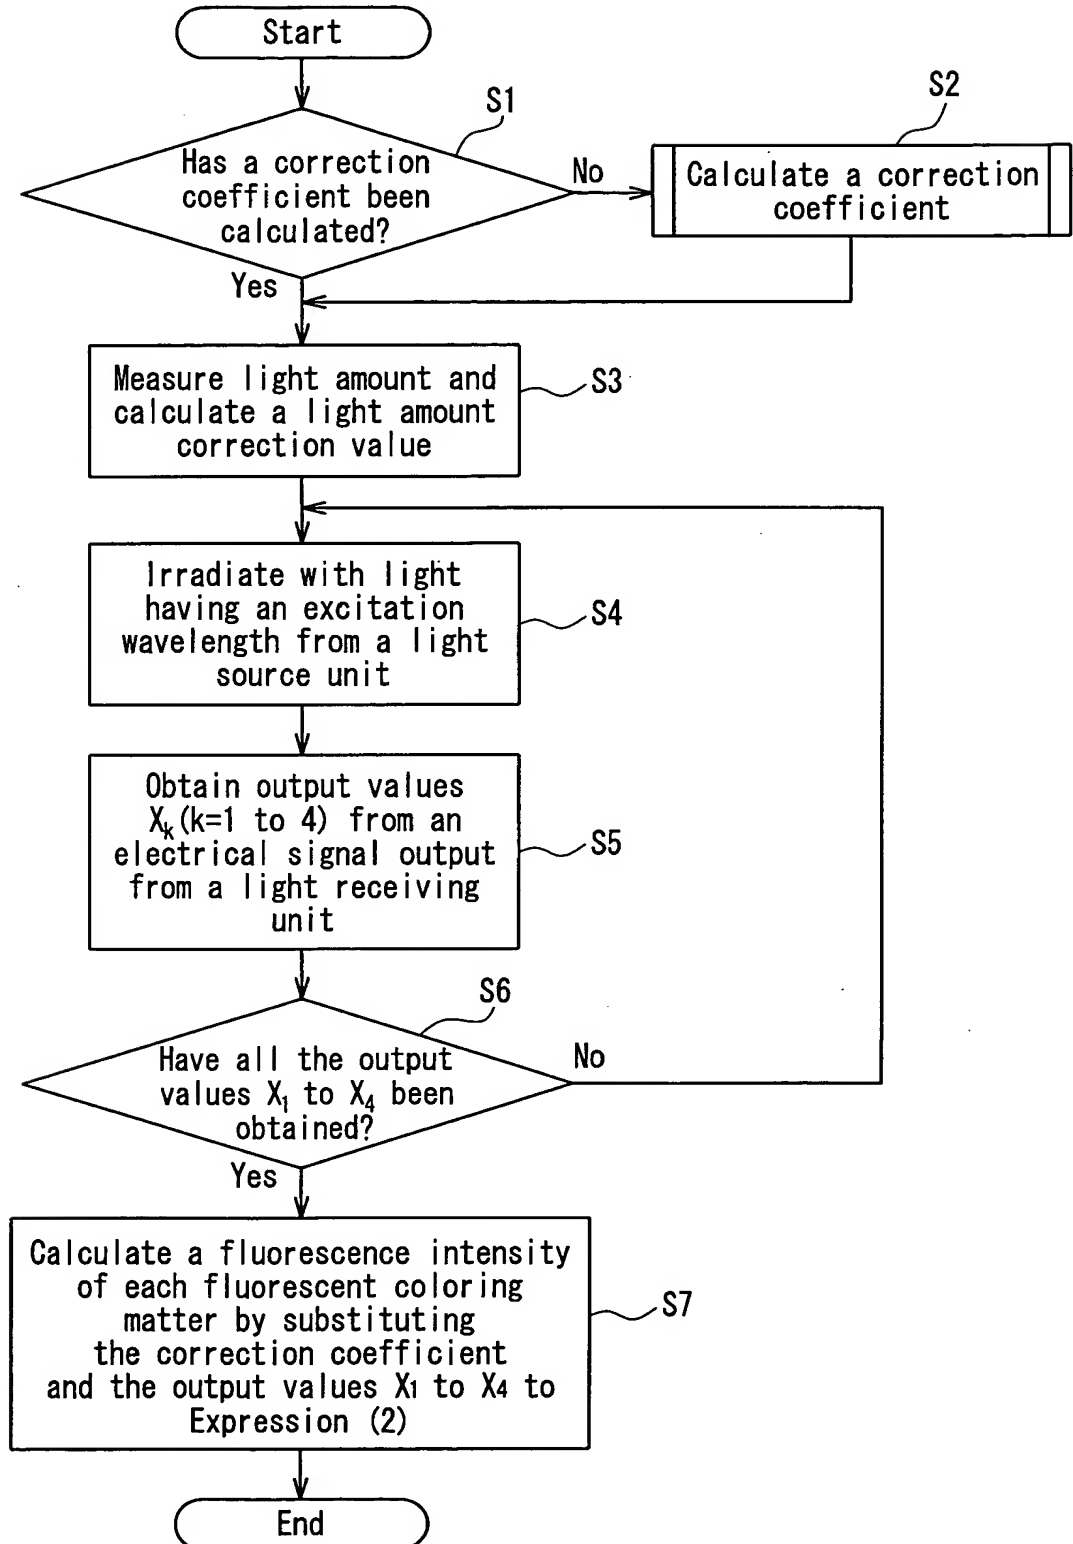


FIG. 2

3/4

Correction coefficient calculation process

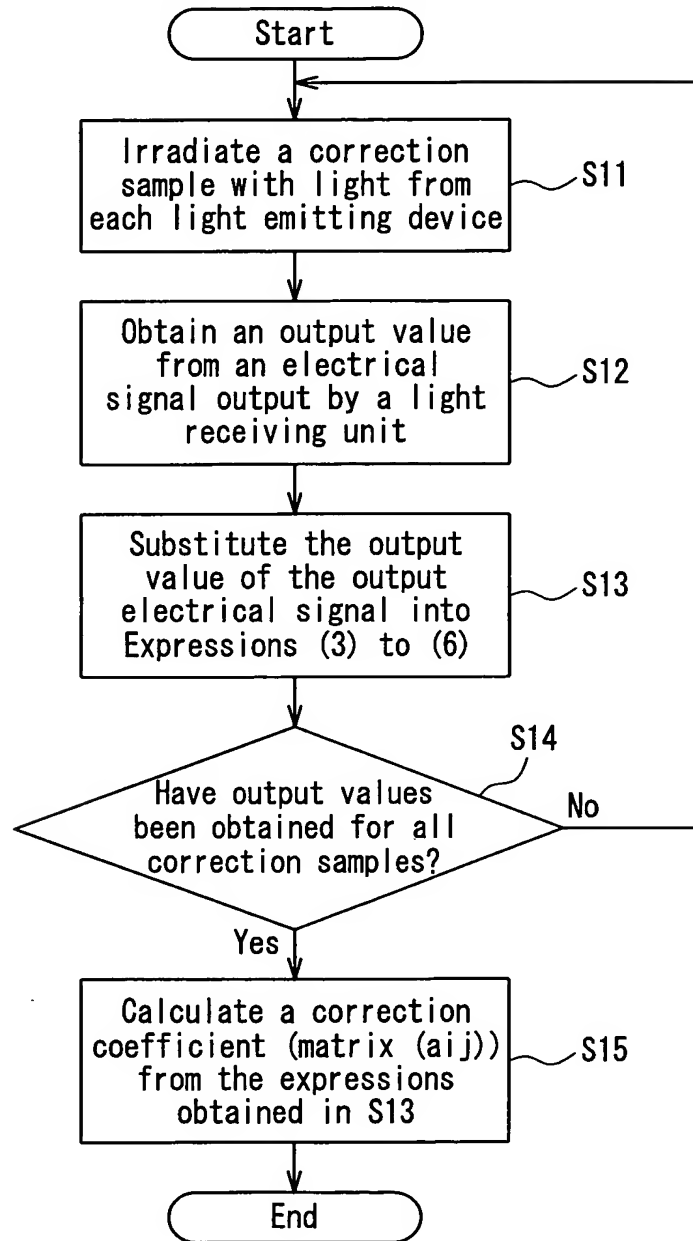


FIG. 3

4/4

Light amount correction value calculation process

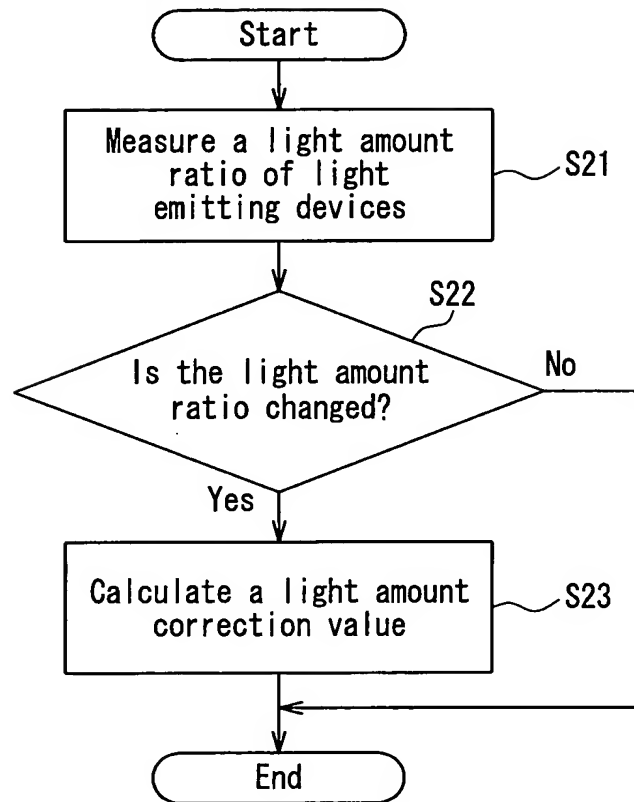


FIG. 4